



# TEST REPORT



No.: WT204030016

Page 1 of 4 Pages

**Sample Description:** Disposable Surgical mask

**Model/Specification/Grade:** MP211/Type IIR

**Applicant:** [REDACTED]

**Applicant Address:** Refer To Next Pages

**Date of Receipt:** 2020-04-26

**Test Period:** 2020-04-26 to 2020-05-14

**Test Location:** Longhua Experimental Base

Shenzhen Academy of  
Metrology & Quality Inspection  
(Stamp)



Approved by:

何行月

Issue Date: 2020-05-15

Signature:

何行月



# TEST REPORT

No.: WT204030016

Page 2 of 4 Pages

## Sample Information:

Sample Description: Disposable Surgical mask

Trade Mark: [REDACTED]

Model/Specification/Grade: MP211/Type IIR

Serial/Batch No. of Sample: MP211

Manufactured Date: 2020-03-14

Manufacturer: [REDACTED]

Manufacturer Address: Refer To Next Pages

Sample Quantity: 100pcs

Sample Description before Testing: Normal.

## Client Information:

Applicant: [REDACTED]

Applicant Address: Refer To Next Pages

Applicant Telephone: -----

Applicant Post Code: -----

## Test Information:

Date of Receipt: 2020-04-26

Applicant No.: 8288142

Environment Condition: (18~25) °C (30~70) %RH

Sampling Method: Delivered by Applicant

Judgment Basis: EN 14683:2019+AC:2019

Test Standard: ISO 22609:2004 and other method standards refer to next pages.

## Test Conclusion:

Test result refer to next pages.

Tested by:

廖惠萍

廖惠萍

Checked by:

刘石磊

刘石磊



# TEST REPORT

No.: WT204030016

Page 3 of 4 Pages

Test Item	Requirement	Test Result	Conclusion
Bacterial filtration efficiency (BFE) (%)	Type IIR $\geq 98$	Sample 1: 100.0 Sample 2: 100.0 Sample 3: 100.0 Sample 4: 100.0 Sample 5: 100.0	PASS
EN 14683:2019+AC:2019, Annex B			
Differential pressure (Pa/cm <sup>2</sup> )	Type IIR $< 60$	Average value: <u>36.4</u> Flow rate: 8L/min	PASS
EN 14683:2019+AC:2019, Annex C			
Splash resistance pressure (kPa)	Type IIR $\geq 16.0$	AQL4.0%, the highest corresponding blood pressure: <u>21.3</u>	PASS
ISO 22609:2004			
Microbial cleanliness (cfu/g)	Type IIR $\leq 30$	Sample 1: 1.0 Sample 2: 1.2 Sample 3: 1.0 Sample 4: 1.2 Sample 5: 1.0	PASS
EN 14683:2019+AC:2019			

Note:

Applicant Address and Manufacturer Address:






# TEST REPORT

No.: WT204030016

Page 4 of 4 Pages

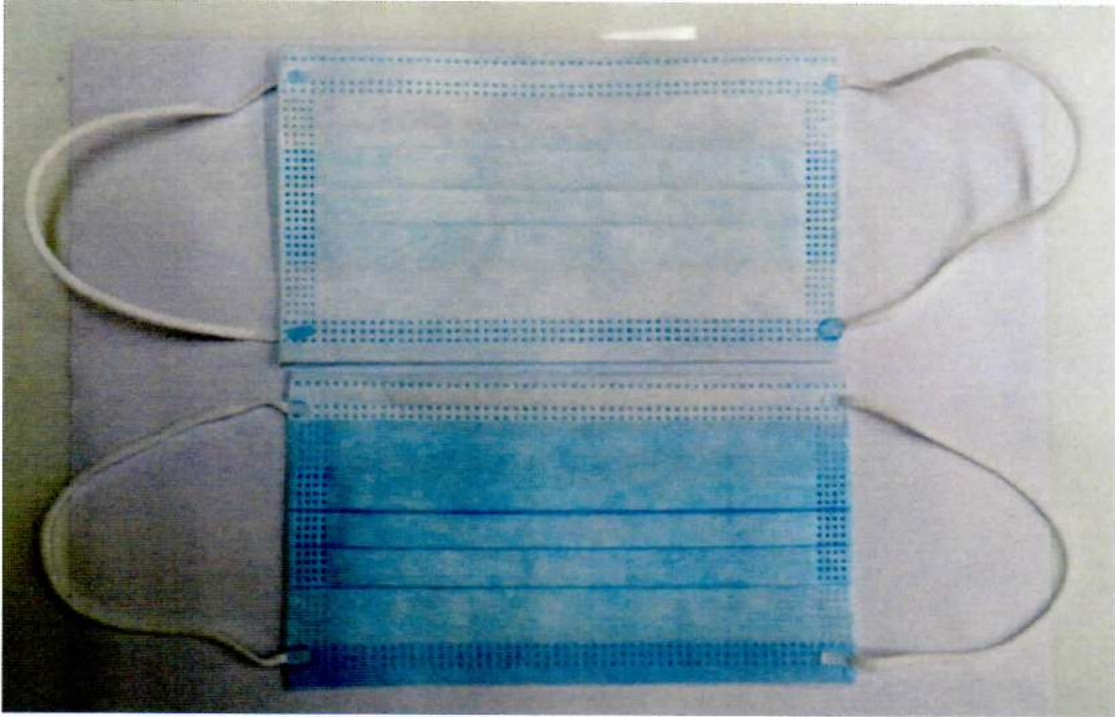

END OF REPORT

